


FIVE YEAR OUTCOMES OF THE PYTHAGORAS US CLINICAL TRIAL

AORFIX 美国临床试验 5年成绩

Shrinkage Rate

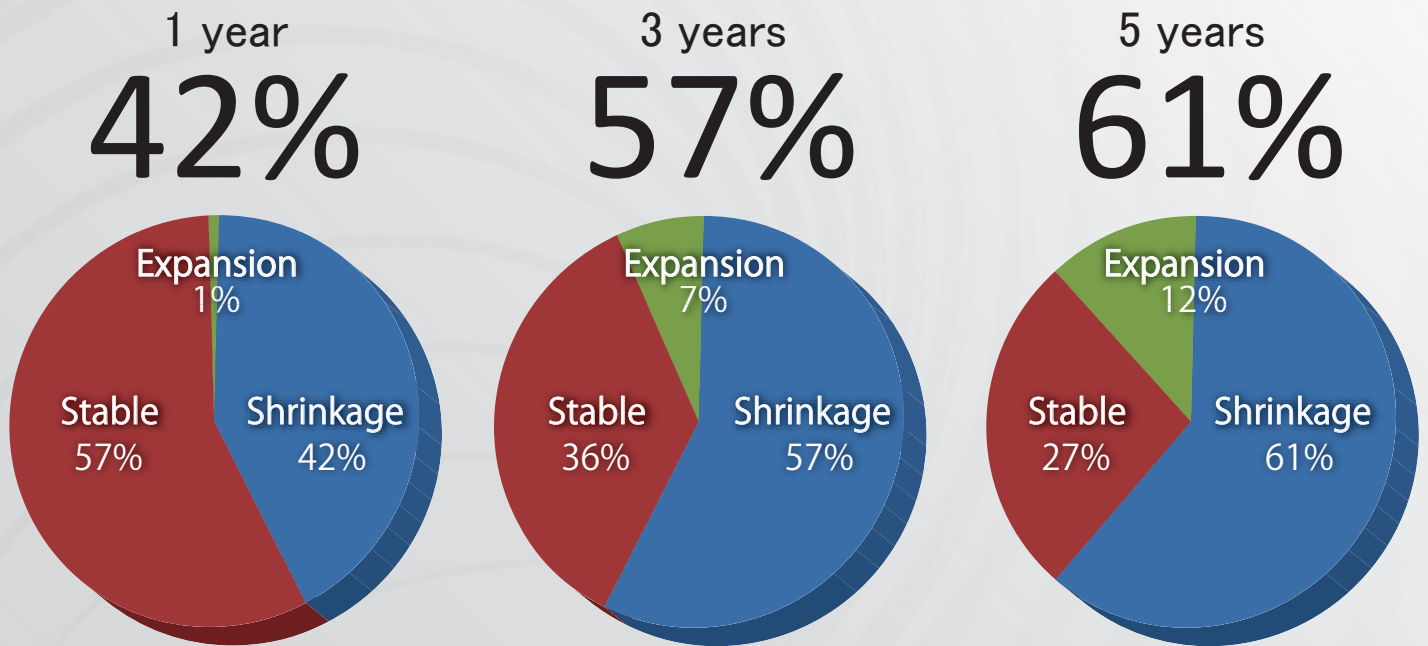

	Total (N=218)			<60 degrees (N=67)			≥60 degrees (N=151)		
	1year	3 years	5 years	1year	3 years	5 years	1year	3 years	5 years
All-cause mortality	7% (16/218)	19% (42/218)	31% (67/218)	6% (4/67)	13% (9/67)	27% (18/67)	8% (12/151)	22% (33/151)	33% (49/151)
Sac shrinkage (>5 mm)	42% (69/165)	57% (74/129)	61% (52/85)	39% (20/51)	61% (26/43)	64% (16/25)	43% (49/114)	56% (48/86)	60% (36/60)
Sac expansion (>5 mm)	1% (2/165)	7% (9/129)	12% (10/85)	0% (0/51)	7% (3/43)	4% (1/25)	2% (2/114)	7% (6/86)	15% (9/60)

FIVE YEAR OUTCOMES OF THE PYTHAGORAS US CLINICAL TRIAL

AORFIX米国臨床試験 5年成績

Endoleaks and Freedom from reintervention

	Type I or III	Type II	Freedom from reintervention
1 year	1%	13%	90%*
3 years	0%	8%	86%
5 years	0%	9%	83%

* 脚注: 引用文献内に誤植があるため正しい数値にて記載

	Total (N=218)			<60 degrees (N=67)			≥60 degrees (N=151)		
	1 year	3 years	5 years	1 year	3 years	5 years	1 year	3 years	5 years
Type I or III	1% (2/149)	0% (0/114)	0% (0/72)	0% (0/46)	0% (0/38)	0% (0/25)	2% (2/103)	0% (0/76)	0% (0/47)
Type II	13% (20/149)	8% (9/114)	9% (7/75)	15% (7/46)	5% (2/38)	11% (3/27)	13% (13/103)	9% (7/76)	8% (4/48)
Reintervention	10%* (22/218)	14% (31/218)	17% (38/218)	8% (5/67)	9% (6/67)	12% (8/67)	11% (17/151)	17% (25/151)	20% (30/151)

* 脚注: 引用文献内に誤植があるため正しい数値にて記載

文献

Malas MB, Hicks CW, Jordan WD Jr, Hodgson KJ, Mills JL Sr, Makaroun MS, Belkin M, Fillinger MF. Five-year outcomes of the PYTHAGORAS U.S. clinical trial of the Aorfix endograft for endovascular aneurysm repair in patients with highly angulated aortic necks. Journal of Vascular Surgery. 2017;65(6), 1598-1607.

販売名: AORFIX AAA スtentグラフトシステム
承認番号: 22600BZX00317000
製造販売業者: 株式会社メディコスヒラタ